

NATIONAL STANDARD METHOD

ONPG (β -GALACTOSIDASE) TEST

BSOP TP 24

Issued by Standards Unit, Department for Evaluations, Standards and Training
Centre for Infections







ONPG (β -GALACTOSIDASE) TEST

Issue no: 2 Issue date: 06.07.10 Issued by: Standards Unit, Department for Evaluations, Standards and Training Page no: 1 of 9
BSOP TP 24i2

This NSM should be used in conjunction with the series of other NSMs from the Health Protection Agency

www.evaluations-standards.org.uk

Email: standards@hpa.org.uk

STATUS OF NATIONAL STANDARD METHODS

National Standard Methods, which include standard operating procedures (SOPs), algorithms and guidance notes, promote high quality practices and help to assure the comparability of diagnostic information obtained in different laboratories. This in turn facilitates standardisation of surveillance underpinned by research, development and audit and promotes public health and patient confidence in their healthcare services. The methods are well referenced and represent a good minimum standard for clinical and public health microbiology. However, in using National Standard Methods, laboratories should take account of local requirements and may need to undertake additional investigations. The methods also provide a reference point for method development.

National Standard Methods are developed, reviewed and updated through an open and wide consultation process where the views of all participants are considered and the resulting documents reflect the majority agreement of contributors.

Representatives of several professional organisations, including those whose logos appear on the front cover, are members of the working groups which develop National Standard Methods. Inclusion of an organisation's logo on the front cover implies support for the objectives and process of preparing standard methods. The representatives participate in the development of the National Standard Methods but their views are not necessarily those of the entire organisation of which they are a member. The current list of participating organisations can be obtained by emailing standards@hpa.org.uk.

The performance of standard methods depends on the quality of reagents, equipment, commercial and in-house test procedures. Laboratories should ensure that these have been validated and shown to be fit for purpose. Internal and external quality assurance procedures should also be in place.

Whereas every care has been taken in the preparation of this publication, the Health Protection Agency or any supporting organisation cannot be responsible for the accuracy of any statement or representation made or the consequences arising from the use of or alteration to any information contained in it. These procedures are intended solely as a general resource for practising professionals in the field, operating in the UK, and specialist advice should be obtained where necessary. If you make any changes to this publication, it must be made clear where changes have been made to the original document. The Health Protection Agency (HPA) should at all times be acknowledged.

The HPA is an independent organisation dedicated to protecting people's health. It brings together the expertise formerly in a number of official organisations. More information about the HPA can be found at www.hpa.org.uk.

The HPA aims to be a fully Caldicott compliant organisation. It seeks to take every possible precaution to prevent unauthorised disclosure of patient details and to ensure that patient-related records are kept under secure conditions¹.

More details can be found on the website at www.evaluations-standards.org.uk. Contributions to the development of the documents can be made by contacting standards@hpa.org.uk.

The reader is informed that all taxonomy in this document was correct at time of issue.

Please note the references are now formatted using Reference Manager software. If you alter or delete text without Reference Manager installed on your computer, the references will not be updated automatically.

Suggested citation for this document:

Health Protection Agency (2010). *ONPG (β -Galactosidase) Test*. National Standard Method BSOP TP 24 Issue 2. http://www.hpa-standardmethods.org.uk/pdf_sops.asp.

ONPG (β -GALACTOSIDASE) TEST

Issue no: 2 Issue date: 06.07.10 Issued by: Standards Unit, Department for Evaluations, Standards and Training Page no: 2 of 9
BSOP TP 24i2

This NSM should be used in conjunction with the series of other NSMs from the Health Protection Agency

www.evaluations-standards.org.uk

Email: standards@hpa.org.uk

INDEX

STATUS OF NATIONAL STANDARD METHODS.....	2
INDEX.....	3
AMENDMENT PROCEDURE.....	4
SCOPE OF DOCUMENT.....	5
INTRODUCTION.....	5
TECHNICAL INFORMATION.....	5
1 SAFETY CONSIDERATIONS.....	6
2 REAGENTS AND EQUIPMENT.....	6
3 QUALITY CONTROL ORGANISMS.....	6
4 PROCEDURE AND RESULTS.....	6
5 ACKNOWLEDGEMENTS AND CONTACTS.....	7
APPENDIX: ONPG (β-GALACTOSIDASE) TEST.....	8
REFERENCES.....	9

ONPG (β-GALACTOSIDASE) TEST

Issue no: 2 Issue date: 06.07.10 Issued by: Standards Unit, Department for Evaluations, Standards and Training Page no: 3 of 9
BSOP TP 24i2

This NSM should be used in conjunction with the series of other NSMs from the Health Protection Agency

www.evaluations-standards.org.uk

Email: standards@hpa.org.uk

AMENDMENT PROCEDURE

Controlled document reference	BSOP ID 24
Controlled document title	ONPG (β-Galactosidase) Test

Each National Standard Method has an individual record of amendments. The current amendments are listed on this page. The amendment history is available from standards@hpa.org.uk.

On issue of revised or new pages each controlled document should be updated by the copyholder in the laboratory.

Amendment Number/ Date	Issue no. Discarded	Insert Issue no.	Page	Section(s) involved	Amendment
2/ 06.07.10	1.1	2	All	Whole document	Document reviewed, reference strains updated

ONPG (β -GALACTOSIDASE) TEST

Issue no: 2 Issue date: 06.07.10 Issued by: Standards Unit, Department for Evaluations, Standards and Training Page no: 4 of 9
BSOP TP 24i2

This NSM should be used in conjunction with the series of other NSMs from the Health Protection Agency

www.evaluations-standards.org.uk

Email: standards@hpa.org.uk

ONPG (β -GALACTOSIDASE) TEST

SCOPE OF DOCUMENT

The test is important in differentiating among the Enterobacteriaceae which are commonly classified according to their ability to ferment lactose. It is also used to differentiate *Neisseria lactamica* from other fastidious *Neisseria* species.

INTRODUCTION

The ONPG (o-nitrophenyl- β -D-galactopyranoside) test is used to determine the presence or absence of the enzyme β -galactosidase in an organism². The presence of two enzymes, permease and β -galactosidase, are required to demonstrate lactose fermentation. True lactose non-fermenters do not possess either of these enzymes. Late lactose fermenting organisms do not have permease, but do possess β -galactosidase which hydrolyses lactose to form galactose and glucose. ONPG is similar in structure to lactose. If β -galactosidase is present, the colourless ONPG is split in to galactose and o-nitrophenol, a yellow compound³.

TECHNICAL INFORMATION/LIMITATIONS

Discard the substrate if it looks yellow prior to inoculation.

Organisms that have grown on glucose containing media show less reactivity than those grown on lactose containing media. Glucose inhibits β -galactosidase.

The test cannot be performed on organisms containing a yellow pigment.

The ONPG solution must be correctly buffered to prevent false-negative and false-positive reactions.

ONPG (β -GALACTOSIDASE) TEST

Issue no: 2 Issue date: 06.07.10 Issued by: Standards Unit, Department for Evaluations, Standards and Training Page no: 5 of 9
BSOP TP 24i2

This NSM should be used in conjunction with the series of other NSMs from the Health Protection Agency

www.evaluations-standards.org.uk

Email: standards@hpa.org.uk

1 SAFETY CONSIDERATIONS⁴⁻¹⁰

Refer to current guidance on the safe handling of all organisms and reagents documented in this NSM.

All work likely to generate aerosols must be performed in a microbiological safety cabinet.

The above guidance should be supplemented with local COSHH and risk assessments.

Compliance with postal and transport regulations is essential.

2 REAGENTS AND EQUIPMENT¹¹

Discrete bacterial colonies growing on solid medium.

ONPG broth (alternatively, commercially available prepared ONPG discs may be used according to the manufacturer's instructions).

Bacteriological straight wire/loop (preferably nichrome) or disposable alternative.

3 QUALITY CONTROL ORGANISMS

Positive control: *Escherichia coli* NCTC 10418 or
Neisseria lactamica NCTC 10617

Negative control: *Proteus mirabilis* NCTC 10975 or
Neisseria gonorrhoeae NCTC 8375

NB Strains not validated by NCTC to give this result

4 PROCEDURE AND RESULTS

- Include positive and negative controls with every batch of tests.
- The test should be performed, where possible, from a non-selective medium. If the test is performed from selective agar, a purity plate must be included to check for purity of the organism.
- Inoculate tubes containing ONPG reagent and incubate at 35-37°C for up to 24 hours.
- Examine for yellow colour after 4 hours and for up to 24 hours.

Positive result: Yellow colour (indicates lactose fermenter)

Negative result: Colourless/pale yellow (indicates lactose non-fermenter)

ONPG (β-GALACTOSIDASE) TEST

Issue no: 2 Issue date: 06.07.10 Issued by: Standards Unit, Department for Evaluations, Standards and Training Page no: 6 of 9
BSOP TP 24i2

This NSM should be used in conjunction with the series of other NSMs from the Health Protection Agency

www.evaluations-standards.org.uk

Email: standards@hpa.org.uk

5 ACKNOWLEDGEMENTS AND CONTACTS

This National Standard Method has been developed, reviewed and revised by the National Standard Methods Working Group for clinical Bacteriology (http://www.hpa-standardmethods.org.uk/wg_bacteriology.asp). The contributions of many individuals in clinical bacteriology laboratories and specialist organisations who have provided information and comment during the development of this document, and final editing by the Medical Editor are acknowledged.

The National Standard Methods are issued by Standards Unit, Department for Evaluations, Standards and Training, Centre for Infections, Health Protection Agency, London.

For further information please contact us at:

Standards Unit
Department for Evaluations, Standards and Training
Centre for Infections
Health Protection Agency
Colindale
London
NW9 5EQ

E-mail: standards@hpa.org.uk

ONPG (β -GALACTOSIDASE) TEST


Issue no: 2 Issue date: 06.07.10 Issued by: Standards Unit, Department for Evaluations, Standards and Training Page no: 7 of 9
BSOP TP 24i2

This NSM should be used in conjunction with the series of other NSMs from the Health Protection Agency

www.evaluations-standards.org.uk

Email: standards@hpa.org.uk

APPENDIX: ONPG (β -GALACTOSIDASE) TEST

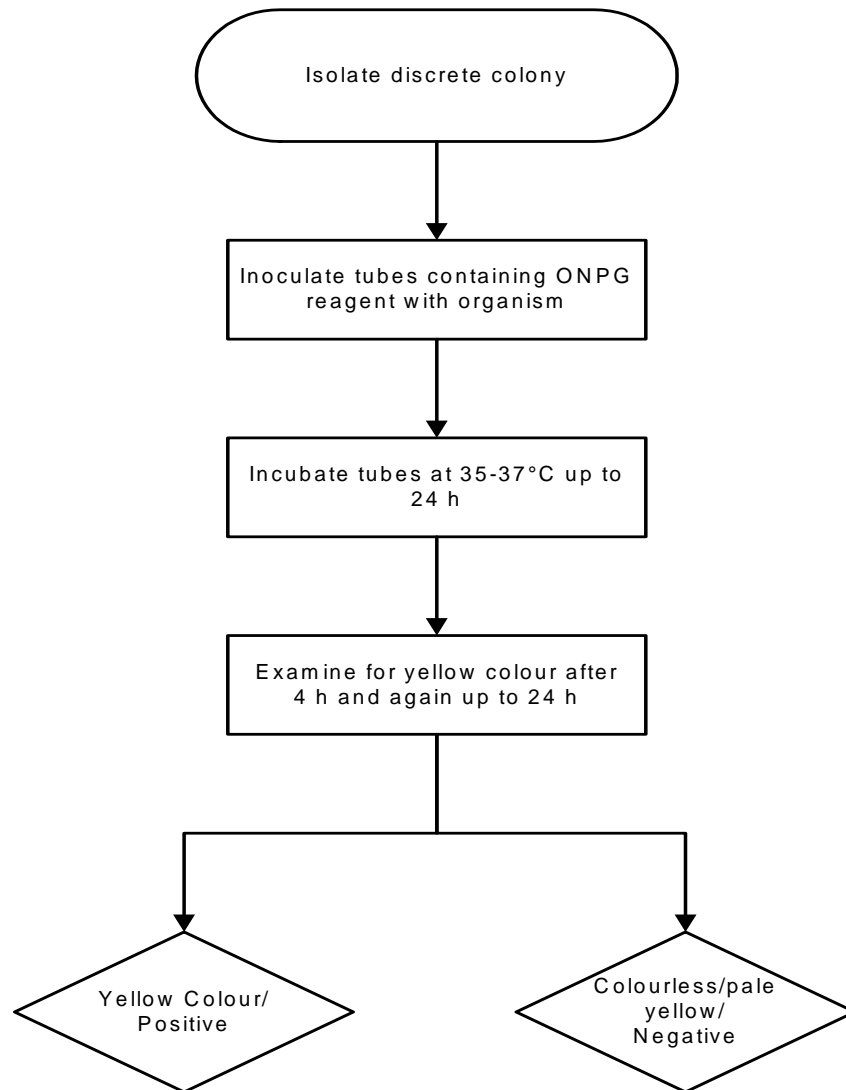

Note:

Positive control: *Serratia marcescens* NCTC 11935 or
Neisseria lactamica NCTC 10617

Negative control: *Providencia rettgeri* NCTC 7475 or
Neisseria gonorrhoeae NCTC 8375

ONPG (β -GALACTOSIDASE) TEST

Issue no: 2 Issue date: 06.07.10 Issued by: Standards Unit, Department for Evaluations, Standards and Training Page no: 8 of 9
BSOP TP 24i2

This NSM should be used in conjunction with the series of other NSMs from the Health Protection Agency

www.evaluations-standards.org.uk

Email: standards@hpa.org.uk

REFERENCES

1. Department of Health NHS Executive: The Caldicott Committee. Report on the review of patient-identifiable information. London. December 1997.
2. MacFaddin JF, editor. Biochemical Tests for Identification of Medical Bacteria. 3rd ed. Philadelphia: Lippincott Williams and Wilkins; 2000. p. 363-7
3. Isenberg HD, editor. Clinical Microbiology Procedures Handbook. American Society for Microbiology; 2004. p. 3.3.2-3.3.2.13
4. Advisory Committee on Dangerous Pathogens. 2004 Approved List of Biological Agents. <http://www.hse.gov.uk/pubns/misc208.pdf>. p. 1-17.
5. Public Health Laboratory Service Standing Advisory Committee on Laboratory Safety. Safety Precautions: Notes for Guidance. 4th ed. London: Public Health Laboratory Service (PHLS); 1993.
6. Control of Substances Hazardous to Health Regulations 2002. General COSHH. Approved Code of Practice and Guidance, L5. Suffolk: HSE Books; 2002.
7. Health and Safety Executive. 5 steps to Risk Assessment: a Step by Step Guide to a Safer and Healthier Workplace, IND (G) 163 (REVL). Suffolk: HSE Books; 2002.
8. Health and Safety Executive. A Guide to Risk Assessment Requirements: Common Provisions in Health and Safety Law, IND (G) 218 (L). Suffolk: HSE Books; 2002.
9. Health Services Advisory Committee. Safety in Health Service Laboratories. Safe Working and the Prevention of Infection in Clinical Laboratories and Similar Facilities. 2nd ed. Suffolk: HSE Books; 2003.
10. Health and Safety Executive, editor. Biological Agents: Managing the risks in laboratories and healthcare premises. 5 A.D.
11. Snell JJS, Brown DFJ, Roberts C, editors. Quality Assurance Principles and Practice in the Microbiology Laboratory. London: Public Health Laboratory Service; 1999. p. 147-8

ONPG (β -GALACTOSIDASE) TEST

Issue no: 2 Issue date: 06.07.10 Issued by: Standards Unit, Department for Evaluations, Standards and Training Page no: 9 of 9
BSOP TP 24i2

This NSM should be used in conjunction with the series of other NSMs from the Health Protection Agency

www.evaluations-standards.org.uk

Email: standards@hpa.org.uk